

Personal Health and Illness Management and the Future Vision of Biomedical Clothing Based on WSN

Ge Zhang, Henan University, China*

Zubin Ning, Institute of Henan Huagong Technology, China

ABSTRACT

It is essential to have a fast, reliable, and energy-efficient connection between wireless sensor networks (WSNs). Control specifications, networking layers, media access control, and physical layers should be optimised or co-designed. Health insurance will become more expensive for individuals with lower incomes. There are privacy and cyber security issues, an increased risk of malpractice lawsuits, and more costs in terms of both time and money for doctors and patients. In this paper, personal health biomedical clothing based on wireless sensor networks (PH-BC-WSN) was used to enhance access to quality health care, boost food production through precision agriculture, and improve the quality of human resources. The internet of things enables the creation of healthcare and medical asset monitoring systems that are more efficient. There was extensive discussion of medical data eavesdropping, manipulation, fabrication of warnings, denial of services, position and tracker of users, physical interference with devices, and electromagnetic attacks.

KEYWORDS

Biomedical, Clothing, Cyber Security, Internet of Things, Personal Health, WSN

INTRODUCTION OF PERSONAL HEALTH AND ILLNESS MANAGEMENT

Personal health information management (PHIM) is the key to illness prevention and treatment. Personal health records and condition-specific health management systems are examples of current patient aids that might aid PHIM components. (Chan et al., 2012). The benefits of a healthy lifestyle include a lower chance of developing several ailments, such as cardiovascular disease, stroke, and diabetes. (Fortino et al., 2014). Joint stability, strength, and stamina are all improved by a wide range of motion, and this benefits the aging body by keeping it mobile, stable, and coordinated. (Ray et al., 2020). They defined three types of self-management: medical management, behavioral management, and emotional management (Darwish et al., 2011). Preventing health issues and lowering the number of doctor's appointments and drugs required are two of the many benefits of taking care of one's health (Fraile et al., 2010). Healthcare expenditures connected with the disease can be greatly reduced if people take better care of themselves. The responsibility for one's health should not fall on the person's shoulders (Bachmann et al., 2012). Health promotion and disease prevention are societal responsibilities whether individuals or communities are ultimately responsible for people's well-being. (Elayan et al., 2017. Here are some tried-and-true methods for improving mood and quality of life:

DOI: 10.4018/IJDWM.316126

*Corresponding Author

This article published as an Open Access article distributed under the terms of the Creative Commons Attribution License (<http://creativecommons.org/licenses/by/4.0/>) which permits unrestricted use, distribution, and production in any medium, provided the author of the original work and original publication source are properly credited.

Go for enough sleep, eat healthily, get outside as much as possible, manage your stress, work out regularly, and cut out harmful vices like smoking and alcohol. (Liang et al., 2016).

Wireless sensor networks (WSNs) can potentially transform our way of life in various ways, including healthcare, entertainment, transport, retail, and other industries, as well as independent care and emergency management. Ambient intelligence is an interdisciplinary idea that combines wearable technologies and sensor technologies with computation and machine intelligence research to address everyday challenges (Alemdar et al., 2010). Elderly populations in wealthy countries are one of today's most pressing issues. According to data from the population, nearly 20% of the world's population will be 65 years old or older within the next two decades (Albahri et al., 2021). As a result, governments and health service providers in these countries must address the dilemma of providing high-quality treatment and service to an aging population while cutting healthcare expenditures (Saleh et al., 2020). Integrating sensors and consumer electronics that may be worn on the body or implanted, people's movements and activities can be monitored as they go about their day. (Sheron et al., 2020). Body sensor network systems can be used for various purposes, including medical monitoring, memory enhancement, home automation, and access to medical records. People with cognitive impairments will benefit from wearable and implanted sensor networks, which will help detect early signs of illness and disease in those most at risk (Li, 2013). These solutions are useful for families where both parents work, the elderly, and those with chronic health concerns.

Patients' movement is restricted, and the current leads and cables further jeopardize their already precarious health in most monitoring systems. (Soh et al., 2015). As a result, sensor networks constitute a vast advance over traditional sensors. An implanted sensor system can monitor physiological parameters without a wireless connection, and many biomedical applications use wireless platforms to collect physiological data (Wu et al., 2018). Other authors built neural prosthetic devices while describing a wireless unrespectable bladder wearable healthcare method. Standardized communication techniques for sensing devices may be required shortly if a piece of hardware can build up a WSN with many nodes within and outside a patient's consciousness that may be predefined or randomly picked. (Abbasi et al., 2016). The next generation of medical systems will use standardized hardware and software designs to accommodate interoperable devices. Some of these gadgets may be put to use by the WBAN unconventionally to keep tabs on people's health. (Rishani et al., 2018).

Healthcare and health delivery are changing quickly due to major cultural developments, technological breakthroughs, and increased medical knowledge. (Gravina et al., 2020). A growing number of older adults more people with disabilities and more chronic illnesses are challenges for countries everywhere. There are new challenges for citizens, consumers, and healthcare professionals to improve health quality and affordability. Those who identify as "health-conscious" are more likely to take measures to improve their well-being. Patients increasingly consider themselves "health consumers" with high standards for preventative care and wellness services such as diet, exercise, and sports management. Previously unimaginable options and solutions are now within reach because of scientific breakthroughs like modules and nanostructures that enable artificial intelligence (AI) technologies, size reduction, power savings, and cheap production. (Cerruela García et al., 2016). Information extraction and administration technologies have benefited from recent developments in wireless and mobile telecommunication and signal processing, human-computer interface (HCI), and navigation.

Rapid progress in science and technology in recent decades has made many things that were once science fiction part of our everyday lives. Simply put, a real-time WSN permeates every facet of modern life. The real-time sensor assists seniors in many ways, including alerts, reminders, and in-depth medical instructions. In an emergency, the real-time sensor also creates a live database that can be shared with loved ones and medical professionals. In addition, it is a practical and thorough tool for keeping tabs on one's health. A sensor is a tiny electronic device that can detect changes in its environment, including but not limited to: motion, light intensity, temperature, magnetic activity, and seismic activity. (Juneja et al., 2016). The information gathered by these sensors might be transmitted

elsewhere for safekeeping until required. This kind of communication allows an increasing number of sensors in a system or network to exchange data in either a wired or wireless method. (Acampora et al., 2013). Recent developments in micro-electro-mechanical systems (MEMS) technology have allowed the creation of small, low-power sensor nodes that might be used to establish a wireless sensor network (WSN). The number of sensor nodes in a WSN may vary anywhere from the tens to the hundreds, and these nodes can be utilized to keep tabs on the whole network with almost any supplementary hardware. (Darwish et al., 2019).

Several new difficulties have arisen for our current healthcare systems, which were developed to deal with emergencies and sickness management: the growing elderly population and the skyrocketing price of medical care (Ometov et al., 2021). The number of people aged 65 to 84 in the United States is predicted to rise from 24 billion to roughly 70 million by 2025 when the eldest members of the baby boom generation retire. There will be 761 million over the age of 65 in the world by 2025, up from 357 million in 1990, resulting from this global trend (Mbunge et al., 2021). In addition, the total cost of well-being care in the United States was \$1.8 billion in 2004, and about a 45 billion people in the country lacked health insurance. Another survey indicated that about a third of working-age Americans, most of who have full-time jobs, provide unpaid care to an older parent or another family member. Healthcare costs in less than a decade are expected to account for about 20% of GDP, endangering the health and well-being economy. Healthcare needs a big change toward more scaled and affordable alternatives. Healthcare organizations need to be restructured to focus on wellness management rather than illness management, and early identification and prevention of disease emerge as a solution to these issues. Protecting sensitive patient data from hackers is essential to maintaining patients' faith in the healthcare system and encouraging them to open up about their health. Constantly updating one's knowledge of the ever-evolving provincial and national privacy regulations. One of the most important pieces of technology in moving toward more proactive and less expensive healthcare is continuous health monitoring via wearable systems. Using a wearable health monitoring system, individuals keep a close eye on their acquired real-time information on vital indicators they stay in top physical and mental shape. In a life-threatening situation, these devices can even notify medical personnel.

Long-term monitoring after an acute incident or surgery may help patients return to full health, and it can also be an essential component of the diagnosing process. With long-term health monitoring, physiological signals may be recorded 24 hours a day, seven days a week. After a myocardial infarction, for example, these alterations serve as an excellent recovery signal. As a further benefit, long-term monitoring can assist ensure compliance with treatment guidelines (such as a regular cardiovascular exercise regimen) or monitoring the effects of medication. In addition, monitors can aid patients in recuperating from knee or hip surgery, stroke rehabilitation, and brain damage therapy, among other things. The paper's main contribution is:

- This study studied wearable and implantable body monitoring systems that provide situational information and alarm systems for aberrant circumstances.
- Discussing personal health care access, food production, and human resource quality has been improved using wireless sensor network-based biomedical clothing (PH-BC-WSN).
- This paper evaluates current research activities and highlights challenges that must be addressed to develop wearable further and implanted smart body sensors to increase the quality of life.
- Summary of recent advances in intelligent monitoring applications for wearable and implanted sensors. As sensor networks in healthcare grow environments, explore the benefits gained and the pressing research questions addressed.

An upcoming section is organized: Section 2: discusses similar work and its corresponding discussion. Section 3: discusses personal health biomedical clothing based on wireless sensor networks (PH-BC-WSS). Section 4: Comparing the results and discussion with an existing method. Section 5 concludes with suggestions for future research.

BACKGROUND STUDY

Sensor communication has been implemented in numerous body area network solutions recently published. On-body WSN layer concerns are a major emphasis of some of these studies, while others are general. On-body sensor data is sent to the sink node without collisions utilizing the system's slotted multipoint-to-point architecture. Beacon signals from a chosen sink node are used to synchronize transmission times. Several methods were used to get the information needed, including manually conducting a document query using key phrases, checking internet resources, and then reviewing the value of each returned part of the information. In each section, they'll go over the methods and techniques.

(Albahri et al., 2021) discussed the academic literature by comprehensively analyzing recent developments in IoT-based telemedicine and healthcare (IoT-THA). Telemedicine classification taxonomy under the Internet of Things (IoT) was provided in this study and reviewed studies in other domains related to that classification. The obtained articles were sorted by the inclusion criteria that were specified. IoT-based healthcare applications have never been mapped in each context's process sequence and definition lifecycle. Researchers and practitioners can benefit from this study's findings since they offer further investigation guidance and relevant data. The ambiguity in IoT-based telemedicine trends was addressed in this study.

(Cavaliere et al., 2021) deliberated the in-depth assessment of the current techniques for countering COVID-19 provided in this paper, along with an evaluation of the technologies employed and the limits of the technologies used. A further benefit of this assessment is that it compares and contrasts various data types, including new technologies, diagnostic methods, and vaccine production platforms utilized in the COVID-19 pandemic. This paper identifies some of the difficulties and drawbacks encountered throughout the systematic review, which helps researchers devise more effective methods for containing and controlling the spread of COVID-19.

(Sezer et al., 2021) discussed the piezoelectric energy harvesting (PEH) presented in this work. They'll go over piezoelectric materials conversion principles and how piezoelectric generators function in more detail. Material advancements in piezoelectric energy harvesting materials based on natural piezoelectricity (PEHM-NP) are proposed. Peripheral applications in several domains, such as transportation and structural engineering; airborne applications; water applications; smart systems; microfluidics; biomedical; wearable and implants, and tissue regeneration are discussed in this article. The piezoelectric energy technology's advances, limits, and possible enhancements are examined. This article summarises a wide range of piezoelectric materials for a clean power supply for wireless electronics.

(Zhanget al., 2021) explored a personal health data center built on Hadoop's big-data (PHDC-HBD) platform, with data synchronization and an independent device helping to consolidate and analyze previously dispersed distributed data. With the characteristics of the Hadoop big data network, the tailored cerebrovascular health information system has been developed to give people individualized health management services and make customer management easier for medical staff. This paper can improve conventional healthcare rehabilitation activities by designing a personalized health knowledge system that allows patients to understand their rehabilitation and treatment status anytime and from any location. All healthcare health data dispersed in impartial medical institutions is stored autonomously.

(Salman et al., 2021) deliberated that E-triage and remote prioritization systems that use machine learning algorithms and sensors are subjected to a thorough assessment of all relevant studies in the field. E-triage and remote prioritization systems that use machine learning techniques in medical architecture (ERPS-MLT-MA) are examined in this paper. This study constructed a cross-taxonomy to uncover telemedicine categories related to machine learning algorithms. With this strategy, researchers can better understand how artificial intelligence and machine learning modernize healthcare systems.

As a result, they've written this detailed analysis to highlight the benefits of current research in trans-disciplinary AI, machine learning, and healthcare services projects.

(Rezaee et al., 2022) discussed the automated technique to diagnose PD from sEMG data. Traditional machine learning and deep transfer learning (DTLA-TML) models were utilized in this study. To produce the discriminative feature vectors, To begin, we used three deep pre-trained architectures: Alex Net, VGG-f, and CaffeNet, to stack the retrieved features. All deep structures are used to counteract over-fitting and enhanced noise resistance, even though there are many-layered features from all three structures. The deep hybrid transfer learning-based PD classification technique has hit 99% in various analysis frameworks. Even though minimum processing was required in the feature building of sEMG signals for PD detection, the proposed model can compete with the current SVM-based pattern.

According to the survey, the current IoT-THA, PHDC-HBD, ERPS-MLT-MA, and DTLA-TML methodologies for diverse privacy and cybersecurity and an increased risk of malpractice lawsuits are flawed. Consequently, personal health biomedical clothing is based on wireless sensor networks (PH-BC-WSN). The study examined new training model techniques to address the concerns stated above.

METHOD

This section describes personal health biomedical clothing based on wireless sensor networks (PH-BC-WSN). One by one, the research topics of the chosen articles were scrutinized, and reviewers aggregated and summarised similar concerns instead of writing them all individually. The structure and organization of the technique structure below provide an overview of their general characteristics.


Personal Health Biomedical Clothing Based on Wireless Sensor Networks (PH-BC-WSN)

In the context of ambient intelligence, wireless sensor networks are frequently cited as a keystone technology. It is possible to get useful information from the environment using low-cost, ultra-low-power sensor networks. Sensor networks can be compared to the human body's sensory system in an intelligent environment. Sensor networks can share data collected with other sensor networks or data collection stations near the sensor nodes. It can keep track of anything from ecosystems and energy generation to building maintenance and upkeep using amenity intelligence sensor networks. Therefore, every proposed application has its own set of needs and restrictions. A particular driving usage, the surveillance of people by wearable and implanted sensors, will be presented to increase the usage of such technologies in healthcare and address new health challenges provided by nature. The current generation of biological sensors and actuators has endless potential for measuring, processing, communicating, and behaving intelligently. Diagnostics, ambulatory care, in-home care, and point-of-need care are possibilities for novel measurements and techniques. There is a high market need for components and nanotechnologies in portable biochips for blood analysis, clinical diagnostics, and non-invasive microsensors in the medical field. Integrating sensing, processing, actuating, and communicating into a single device is no longer "wishful thinking." Instead, it is becoming a reality. These technologies are being transformed into body sensor networks due to the rise of WSNs for medical applications.

For example, biosensors can capture electrocardiography, myocardial infarction, and electrodermal activity. For example, heart rate, movement, and even muscular activity can all be detected with accelerometers. Understanding the human body better requires a sensor system that constantly monitors a variety of health markers. The network incorporates numerous networks and wireless devices to provide monitoring systems in a wide range of contexts. When it comes to BC-WSN s, one of their primary uses is in healthcare settings, where the health of many patients is continually being monitored in real-time. WSN deployment in healthcare facilities necessitates wireless monitoring of multiple patients' vital signs simultaneously. Providing biosensor data and the ability to continuously


monitor health factors such as body temperature, heart rate, and blood volume discreetly and efficiently is one of the key purposes of WBANs.

Figure 1. A basic healthcare WSN application scenario

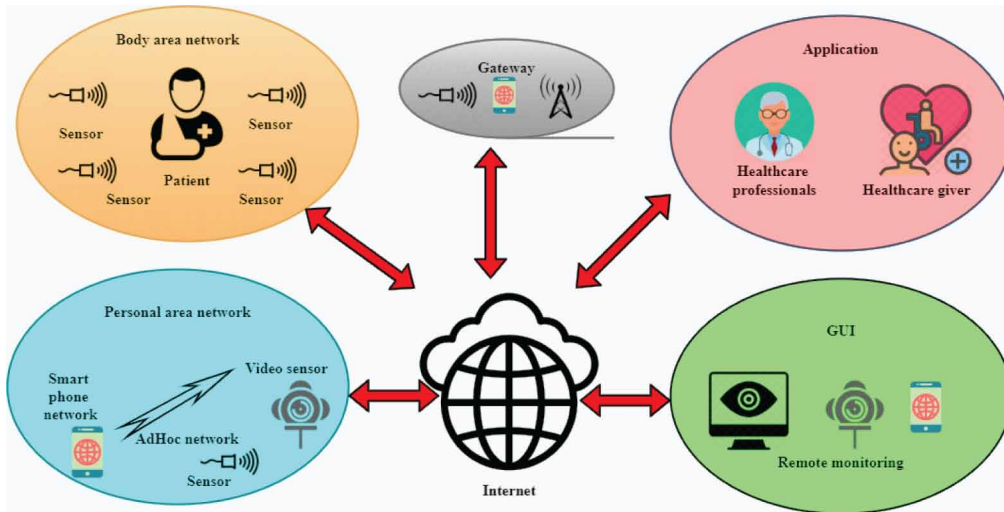

In addition to the commercial items, there are other prototypes. When several apps are examined, it is found that they all share several characteristics. BANs and PANs are two types of sensor networks that have been proposed in the past. BANs consist of sensors carried by the patient, whereas PANs consist of sensors put in the environment (PAN). Gateway nodes connect these two to the backbone network. For healthcare practitioners or other providers patients' vital signs should be closely monitored vital health data in real-time (GUI) using a graphical user interface. During an emergency, the application will generate alarm messages which, together with other health-related data, can be accessed on mobile devices such as laptops, PDAs, and smartphones. Pictured here is one possible use for a simple wireless sensor network, as shown in Figure 1. For example, There are typically four categories of non-powered users in any given system, including administrators, programmers, and system administrators: Children are young people who are unable to care for themselves, such as newborns, infants, and toddlers, and those who are older but still require continual supervision. It is the role of careers to provide support to those who need it most, including the elderly and chronically ill. Professional caregivers, such as doctors and other medical staff, monitor the health of the elderly and chronically ill and are prepared to respond quickly in an emergency. They are referred to as healthcare professionals.

Figure 2. Wearable smart clothes are incorporated into the system's architecture

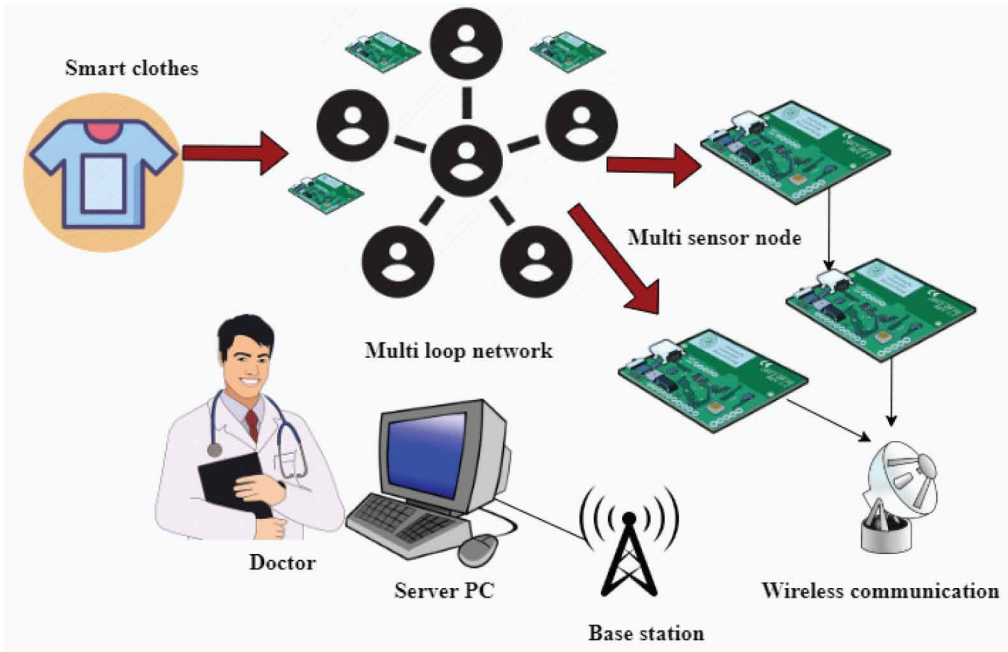

It is now possible to monitor the health of the elderly or the wearer of a smart health monitoring system. An EKG, especially having heart rate, heart rate, core temperature, and physiological signals (GSR) surveillance system termed the 'Smart Vest,' has been created. There are three main components to this wearable smart shirt system: monitoring system components include a sensor network, a wireless device, and a server computer integrated into the node (Figure 2). A smart shirt was designed and created for active surveillance and real-time healthcare. Wearable sensors and conductors in the shirt act as electrodes to record the wearer's bodily impulses. ECG and physical exercise data are sent to a server PC through an ad-hoc network for remote monitoring. Physiology data such as electrocardiography, pulse rates, heart rates, and skin temperatures can now be monitored via a wrist-worn wearable medical surveillance device.

Figure 3. The present use of healthcare sensor networks in the healthcare sector


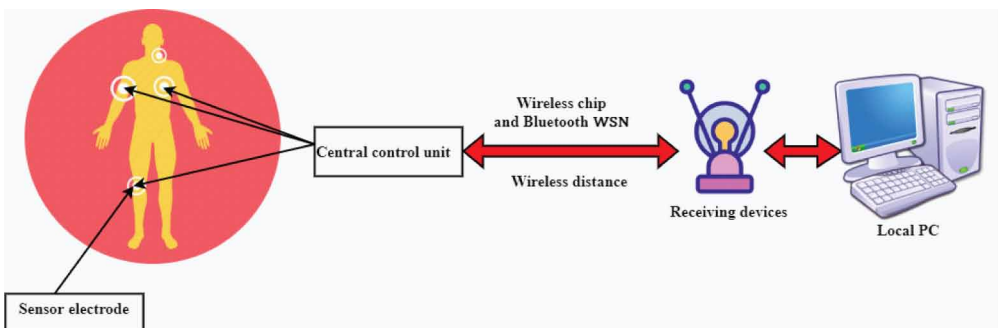


Figure 4. Wireless body area networks used to target healthcare sensor networks

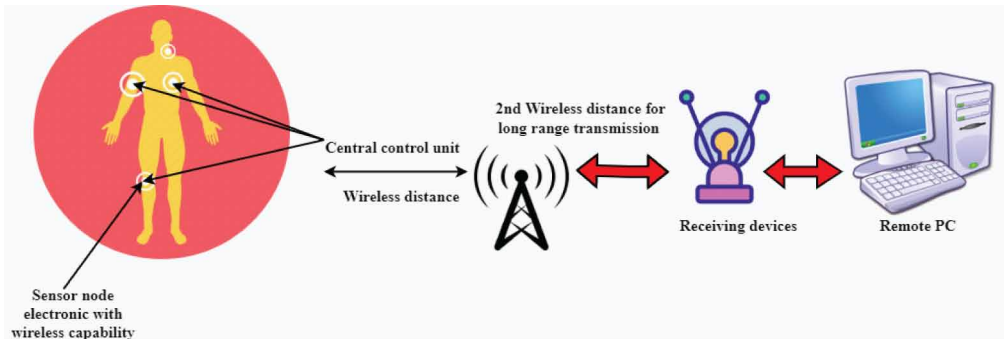

Depending on the specific application, they might be single- or multi-point sensors. Multiple on-body sensors can be used to disperse a person's posture detection. Still, other uses, such as keeping track of patients (see Figures 3 and 4), require all sensors to route dynamic data routing to a sink node, which can then wirelessly transmit the data to an out-of-body server in figure 3. Real-time and non-real-time data transactions are both possible. Even while patient monitoring programs require real-time packet routing, offline processing and analyzing an athlete's physiological data are possible. Wireless sensor networks (WSNs) are proposed in this research for use in continuous patient monitoring. This research introduces a hierarchical addressing structure and a WSN architecture built on gateway trees. This design enables routing in WSNs without the need for route discovery. Because a mobile network is always associated with its home address, it is not necessary to set up a care-of address at any point in the mobility process, eliminating any potential for communication interruption due to an address change. In the suggested system, doctors can track their patients' whereabouts and keep tabs on their health no matter where they are. This allows for more precise diagnosis and faster, more precise treatment. Simulation data suggest that the approach can reduce communication latency and control costs and lower the packet loss rate. Gait cycles are identified using the local peak and valley detection method's accuracy decreases with increased walking speed and changes in gait pattern. Sensors, management electronics, and wireless transceivers are components of a conventional wireless body area network. Compact, light, environmentally safe, and long-lasting power sources are required for these components and are vital to the entire system.

With fewer nodes and less area covered than traditional WSNs, WBANs offer less chance for redundancy. A typical WBAN has between two and 10 nodes, used in various ways. Scalability might lead to inefficiencies. If a BASN's goal is to keep its form aspect and resource utilization as small as possible, adding redundant sensors and paths to the network won't be an option. WBANs are structured hierarchically as well. Microprocessors must process large amounts of data continuously and naturally from their collected data. A hierarchical approach to data processing is important to take advantage of the imbalance of resources, preserve method competence, and confirm the volume of information, if essential.

Figure 5. Healthcare systems often have four-layer architecture


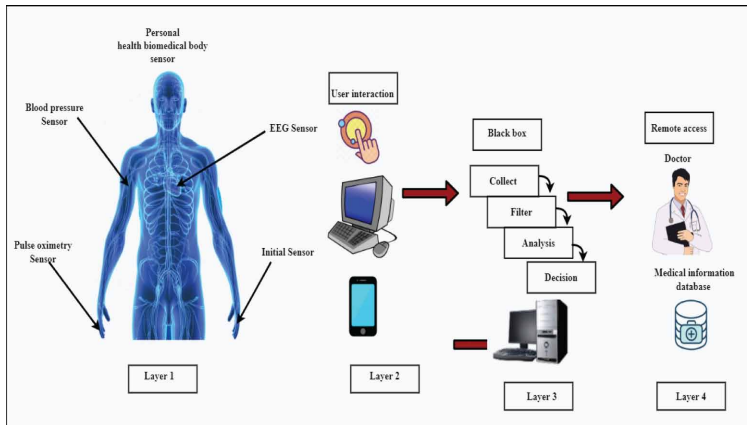


Figure 5 depicts a typical healthcare system design for a home environment. Further explanations of this architecture are provided below. Layer 1 is a personal health biomedical body sensor comprising several sensor nodes communicating over a wireless network. It is possible to sew sensors into clothing or have them implanted under the skin using this layer’s sensor nodes, which are small enough to be applied to the body as patches (on-body sensors). Sensors of this type are constantly gathering and transmitting critical information. Nodes’ capabilities and features reduce overall on-tag processing before transmitting data. Once analyzed, the data is either routed back down to the lower levels of the body or processed by a body coordinator. The amount of power a sensor node consumes in an off-body communication depends on several factors, including the body path loss (BPL), receive noise figure (RNF), and signal-to-noise ratio (SNR). For BPL, antenna radiation patterns are extremely important. Devices affect RNF, and A unique RNF identifies each device, which is found in the datasheet. However, the overall quality of the communication channel affects SNR.

Figure 6. Develop smart biomedical clothes disciplines involved

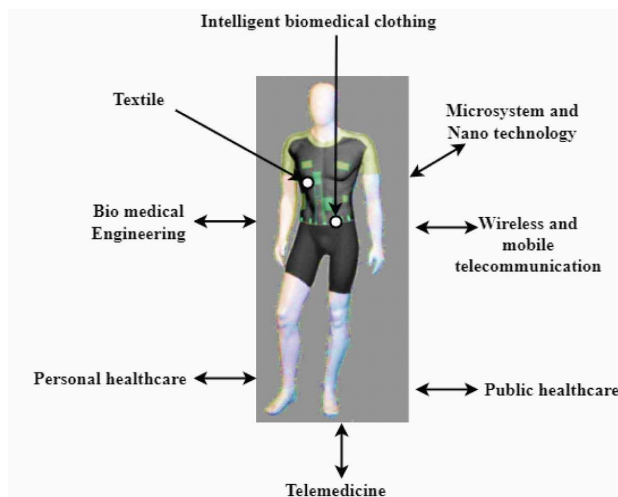

With Bluetooth or Wi-Fi, smart garments may pair with mobile applications or secondary devices like laptops and PCs. These high-tech garments are equipped with sensors that can measure a wide range of biometric data, making it possible to track things like location, speed, elevation, core body temperature, blood oxygen saturation, and much more about physical activity. The information is sent to smartphone applications that use artificial intelligence to improve health and productivity. The term “wearable technology” refers to any electronic device worn on the body to collect data or provide service. Smart watches, smart jewelry, fitness trackers, smart shoes, smart belts, brain activity monitors, etc. are just a few of the many kinds of wearable technology presently used to keep tabs on our bodies and their functions. As part of a multi-disciplinary effort, IBC is being developed by engineers and scientists from a wide range of fields, involving mobile and wireless telephony and nanotechnology as well as textiles and apparel (Figure 6). “Citizens’ health clothes” are taking the place of “patients’ medical apparel” in the conceptual hierarchy. A combination of currently available tools and sensors on common apparel could lead to medical gear that is disproportionately large. Sensors built into medical equipment are used to raise the quality of care provided to patients, increase their comfort level, boost the efficiency of medical staff, and lower healthcare expenses. In terms of the patient, advantages include the following: During medical procedures, patients often benefit from being put to sleep by using an anesthesia machine.

As a result, people may use their mobile devices to quickly and reliably get up-to-date health information. These applications make it simple for patients to schedule doctor’s visits, get timely reminders, and see their lab results. As a result, healthcare will benefit from next-gen sensor technology since it will provide more direct communication between patients, medical professionals, and treatment options. Pre-commercial prototypes, such as pajamas to identify Sudden Infant Death Syndrome³⁷ or products, already accomplish this today. The Life T-Shirt, for example, provides ambulatory respiratory monitoring and heart rate variability in real-time. These garments are meant to be worn for medical reasons, and technology like infrared sensors and wireless networks should be incorporated. For this to happen, extensive study and experimentation would be required. A source of power is needed to integrate sensors and actuators. A person’s clothing can act as a source, a processor, and a means of communication. Current generation prototypes like “medical aid” and “smartshirt^{TM39}.”

Further validation work in the medical field is needed for the “VTAMN Project.” a deeper dive into the issue of creating “e-textiles” is the goal of new fiber materials. There are three main components in today’s world of information technology: Physiological and biomechanics signals are monitored as elements of a weaving framework. For IBC to succeed, the engagement and acceptance of healthcare providers are essential. Both the government and third-party payers are responsible for this debt. As soon as the project began, we considered all the financial aspects of the services. Health experts and insurance firms are working together to establish new business models.

Patients at greater risk may remain at home with a monitoring system, which frees up resources and hospital beds for other patients. As a result, hospitals and other medical centers may save money and run more efficiently by ensuring patients in urgent situations get aid quickly. Claims processing may benefit from smart technology’s ability to simplify operations, save costs, and speed up responses. Medical expenses may be reduced and service levels improved because of the technology’s ability to streamline data collecting and communication procedures and provide concrete evidence of what transpired to warrant a claim.

This research is an improvement produced to measure and analyze the real-time medical information confined in the permitted region by modeling WSN. It uses wearable health sensors, including electrocardiograms (ECG), blood pressure monitors, and glucometers). The bounded remote monitoring system, a proprietary wireless sensor network-based biomedical clothing (PH-BC-WSN) environment created to evaluate patients’ health, collects real-time medical data inside the hospital’s boundaries. A novel wireless sensor network scenario has been devised and built to store or track patients’ health data round-the-clock. This study provides a fresh, protected vantage point from which

to view the expansion of patient access to their medical records and the subsequent improvement of healthcare infrastructure.

Personal Health and Illness Management

Biomedical apparel powered by wireless sensor networks as a tool for monitoring and managing mental well-being and disease: a look at the present and future. Compression reduces the quantity of data being transferred, and network efficiency and improved power results were achieved through compression. Sensors such as ECG, EEG, SpO2, temperatures, and altimeter (fall detection) are the most commonly used in WSNs. Attempts have been made to reduce the quantity of ECG data since it consumes a great deal of bandwidth, and compression methods may be roughly split into two camps: those that are efficient and those that are not.

In contrast to loss compression techniques, lossless compression methods do not enable any information to be lost in the reconstructed signal. Because WSNs nodes are battery-powered, lossless compression algorithms typically demand more computation and bandwidth, making them incompatible with WSNs. How well compression works may be measured by comparing the number of bits needed to represent the original signal with the number of bits utilized in the condensed signal. Calculating a mistake's root-mean-square difference (PRD) percentage is easy with Equation 1:

$$PRD = \sqrt{\frac{\sum_{j=1}^m [Y_{org}(j) - Y_{rec}(j)]^2}{\sum_{j=1}^m Y_{org}^2(j)}} * 100 \quad (1)$$

Here are some examples of the reconstructed and original data that are Y_{rec} and Y_{org} , respectively.

WSN monitoring provides statistics numerical simulations in the 430–611 MHz and UWB (3.1–10.6 GHz) bands. These statistical channel models compare the performance of several wireless technologies in WSNs in terms of path loss. Both a path loss model and a power delay profile (PDP) stochastic channel model were discussed in this paper. A vector network analyzer was used to calculate the path loss for each frequency band (Equation 2), and a transfer function among two body-worn antennas was obtained (VNA). The typical bandwidth of WSNs, excluding this band, is less than 10 Mbps, indicating that one symbol's transmission length is larger than 30 m:

$$M_{path}(e, g) = b(g) \cdot \log_{10} e + c(g) + o(eC) \quad (2)$$

As shown in equation (2) pathway cost has been utilized. $M_{path}(e, g)$ refers to the pathway cost in eC at the given distance and frequency range. The average route loss derived from the measured is used to determine coefficients $b(g)$ and $c(g)$. According to equation 3, PDP in the ultra-wideband model:

$$i(u) = \sum_{m=0}^{M-1} b_m \exp(k\varphi_m) \delta(u - u_m) \quad (3)$$

Equation 3 shows the power delay profile ultra-wideband model that has been described. The intensity of a message obtained over a multipath channel is represented as a function of delay time by the power delay profile (PDP). The delay results from the different amounts of time it takes for each multipath arrival. In the case of multi-path transmission, the power utilization of the received data is expressed in terms of the delay concerning the initial arrival path, which is known as the power

delay profile of the channel. Due to the many pathways that signals take while being broadcast in WBANs, the network output appears to consist of a sequence of pulses. Where pathway amplitude, entrance period, and stage of the M_{path} the path is denoted by b_m , u_m , and φ_m , respectively. $\delta(u)$ is the dirac function, and m denotes the number of possible arrival pathways. It is possible to express the Cramér mathematically–Rao lower bound (CRLB) as the model-based received signal strength technique’s positioning error:

$$\rho_{CRLB}^2 \succeq \sum_{j=1}^o \frac{1}{e_j^2} / c \left(\sum_{j=1}^{o-1} \sum_{i=j+1}^o \sin^2(\varphi_j - \varphi_i) / e_j^2 e_i^2 \right) \quad (4)$$

Equation 4 shows CRLB) as the model-based received signal strength technique’s positioning error has been calculated. The $c = (10o / \rho_{CRLB}^2 \ln 10)^2$. There are two ways to express this: ρ_{CRLB}^2 signifies a standard deviation of the noise, and o denotes path loss. The distance between the device in an unknown location $\sin^2(\varphi_j - \varphi_i)$ and $e_j^2 e_i^2$ the base stations at known locations (ρ_{CRLB}^2) is denoted base station’s angle of inclination concerning a reported position calculated using the following formula: $\sin \varphi = e^j - e^i$.

It is possible to filter the original fingerprinting dataset using CRLB as the model-based receiving transmit power technology’s placement inaccuracy since it considers the closeness of RSS fingerprints to BLE devices. A tiny subset of all the different types of user positions is used as the foundation for the final user information related. The suggested technique can rapidly estimate location thanks to using a portion of the original fingerprint dataset concurrently improving positioning accuracy by reducing the number of calculation mistakes. The time of arrival placement method’s CRLB is provided as follows:

$$\rho_{CRLB}^2 \succeq 1 / 8\pi^2 \beta \alpha^2 \quad (5)$$

Equation 5 shows the β represents the receiver’s signal-to-noise ratio and α the system’s bandwidth. The positioning error is lower bound inversely proportional to the system bandwidth. Furthermore, the error signal is bandwidth-dependent due to a need to accurately measure the propagation time between transmitters and receivers in the face of unfavorable fading. As a result, the idea of ultra-wideband (UWB) systems for precise localisations is born:

$$\rho_{CRLB}^2 = \int_{-\infty}^{\infty} |Y(g, o, u_q)|^2 eg / O\beta \int_{-\infty}^{\infty} g^2 |Y(g, o, u_q)|^2 / eg \quad (6)$$

Equation 6 shows g is the frequency, u_q is the scaling factor of time, $Y(g, o, u_q)$ is the Fourier transform of $y(g, o, u_q)$ and o denotes specifies the order in which differences are compared, O symbol-period pulse is observed in the observation period, β Figure 7 depicts the signal-to-to-noise ratio (SNR). The CRLB was recalculated to determine the upper limit of the positioning error, as stated explicitly earlier:

$$\rho_{CRLB}^2 \succeq 6(1 + M_\beta) / \pi^2 MO\beta^2 \quad (7)$$

As a lower bound on the variability of an approximate estimate, the Cramer-Rao Lower Bound (CRLB) is a useful tool. In general, estimators closer to the CLRB tend to be more objective than those farther away. They used the Laplace transformation to get closed-form formulas for the CRLB. The CRLB decision is complex to analyze, calling for familiarity with mathematics and probability theory. Equation 7 shows M is the number of sensors, O is the length of the measurement vector. For the most accurate localization, SNR (denoted by) and the number of receivers (M) are critical considerations, as shown in equation (7). The following is the CRLB for an angle of arrival system operating in line-of-sight:


$$\rho_{CRLB}^2 \geq OS^2 \rho^2 / \sum_{j=1}^{O-1} \sum_{i=j+1}^O \sin^2(\varphi_j - \varphi_i) \quad (8)$$

Equation 8 shows $\sin^2(\varphi_j - \varphi_i)$ is the difference in angular orientation between two adjacent receivers, S is the estimated separation between the receiving and the receiver's actual location, O the total number of recipients, ρ is the received noise standard. The determination of the WSN telecommunication program's assessment of the cascading channel.

When the combined typicality-based connection estimation method is utilized, the MSE of assessment can monotonically accomplish the CRLB as the good or service of the multitude of transceiver antenna elements and the quantity of time slot machines tends to infinity. Additionally, this bound can be monotonically achieved regardless of whether the estimator knows the locations of the non-zero submissions in the stream.

Finally, the security ratio, behavior analysis ratio, tracking rate, expensive rate, specificity ratio and precision ratio were all considered. According to this study, personal health biomedical clothing based on wireless sensor networks (PH-BC-WSN) compares survey findings with other studies.

Figure 7. Signal-to-noise ratio (SNR)

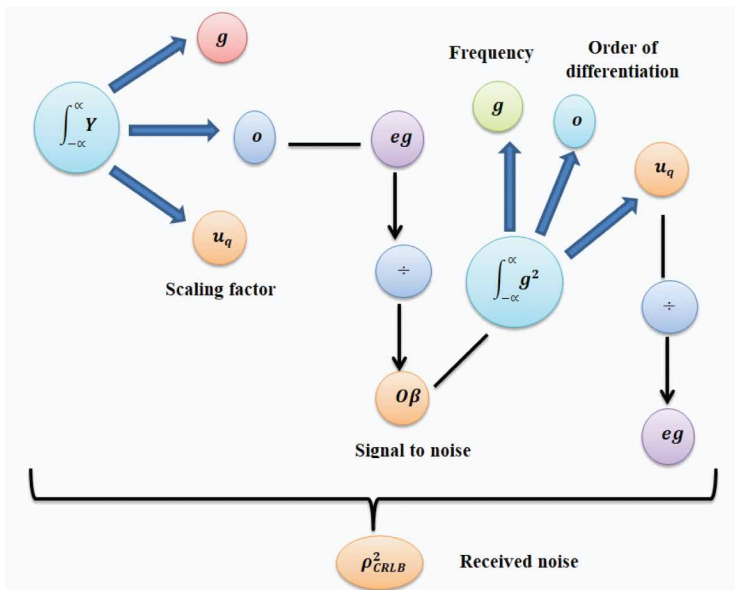

RESULTS AND DISCUSSION

Challenges arose throughout the building of ubiquitous healthcare systems, and this section outlines some of the unanswered research topics that emerged. Many issues exist at each stage of the wireless sensor network. In this survey, we take a healthcare-specific approach to these issues. The issues listed above must be addressed for wireless sensor networks in healthcare to provide their full potential. Several technological and medical concerns need to be resolved to conduct clinical trials. Producing greater conductivity textiles using current industrial techniques and interfacing and protecting electronic components are two of the most difficult tasks. Problems with cleaning and washing must be addressed in addition to these difficulties. Other investigation areas include signal processing, interpretation of data, user acceptance, economics, adaptability of products, market analysis, and business model formulations. The benefits mentioned above will be included in the multi-modal sensing technologies that will be used in the future of smart home settings. However, implementing ubiquitous, context-aware healthcare systems is still a challenge. From a healthcare viewpoint have analyzed these issues. Context-aware, pervasive healthcare systems will become accessible to the general public through several sensing modalities such as video sensing, RFID, medical sensors, and smart appliances with remote monitoring capabilities. Analytics increase accuracy, allow early diagnosis, enable personalization, and save costs by decreasing expensive unneeded lab tests. We investigated security, behavior analysis, tracking, expensive, specificity, and precision as the most critical metrics. It was shown that understanding personal health biomedical clothing based on wireless sensor networks (PH-BC-WSN) has compared to earlier research.

Table 1. Comparisons of Performance metrics

Parameters	IoT-THA	PHDC-HBD	ERPS-MLT-MA	DTLA-TML	PH-BC-WSN
Security ratio (%)	45.7	55.67	65.6	47.7	92.11
Energy efficiency ratio (%)	55.6	50.5	65.4	67.8	89.9
Behaviour analysis ratio (%)	62.3	52.3	42.3	64.3	95.23
Tracking rate (%)	23.5	43.5	53.5	25.5	96.8
Specificity ratio (%)	58.5	38.5	68.5	57.5	93.51
Precision ratio (%)	58.5	38.5	68.5	57.5	96.8

An example of industry-wide comparability is seen in table 1. The overall objectives can be better supported if the measurements used to calculate them fall within a certain range. Metrics are used to assess how well employees are performing and whether or not their goals have been met. It is possible to establish whether or not a method meets the needs of its users by analyzing metrics. When transforming client needs and operational successes into comparable data, metrics are essential. Both measures and what they signify are essential to making informed decisions. Put another way, metrics are essential because they turn consumer and operational needs into data.

Precision Ratio (%) and Specificity Ratio (%)

Figures 8 and 9 show that the PH-BC-WSN consumes the largest precision value (98.68%) compared to IoT-THA, PHDC-HBD, ERPS-MLT-MA, and DTLA-TML, which all consume precision values in the range of 96.8%. Healthy persons have been monitored through an efficient training and analysis system. Wearable medical monitoring systems are developed using recall measures. WSN-enabled healthcare data and health monitoring-based machine learning algorithms are used in place of

other classifiers that require less precision. With the PH-BC-WSN method, choosing critical health information is a breeze. As part of improving health monitoring, the system now includes PH-BC-WSN. When it comes to protecting user data, the next generation of communication technologies is still in its infancy. Due to the prevalence of machine learning, there is a pressing need for further study the robustness and safety of wireless systems. A machine learning network with great performance is one of the most promising approaches to strength training data.

Figure 8. Precision ratio (%)


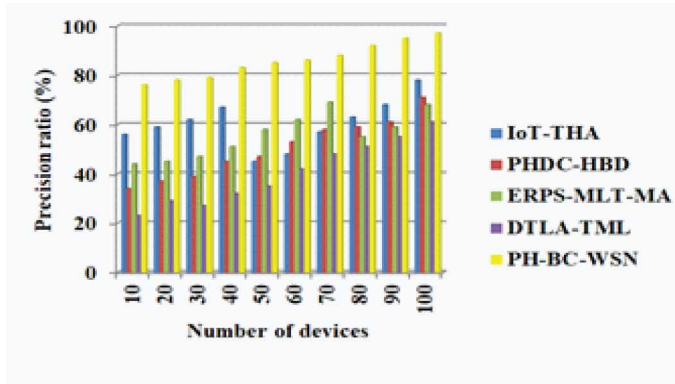


Figure 9. Specificity ratio (%)

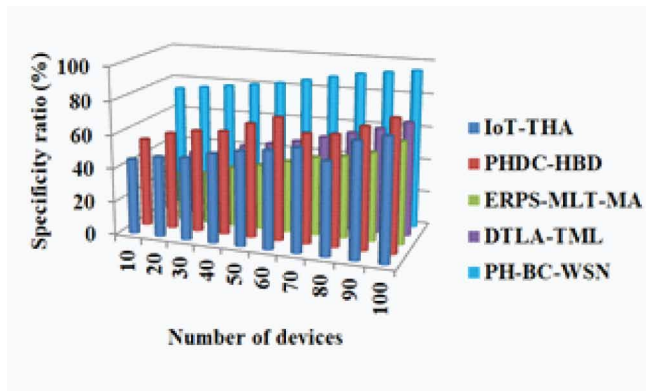

PH-BC-WSN experimental study ensures up to 98.7% precision in testing the system’s effectiveness. Figure 8(b) shows that the most critical factor in assessing physical well-being is the specificity ratio %. PH-BC-WSN methods are used to implement the WSN strategy. PH-BC-WSN enhanced the IoT-THA, PHDC-HBD, ERPS-MLT-MA, and DTLA-TML even though a comparison shows higher performance. Because it uses sequential computational approaches, the proposed solution outperforms standard algorithms in terms of accuracy over a greater number of repetitions. This, however, poses several important challenges, including the cost of computation, the complexity of the method, and the declining gradient. It is expected that these issues will be addressed shortly. The healthcare industry has seen a considerable transition due to the PH-BC-WSN. Real-time analytics

have necessitated greater responsiveness and accuracy in using health monitoring systems. These delays, however, result from poor network connections and the unpredictable nature of sensor data. A massive amount of data is gathered from pertinent sensors. After then, the information is sorted and archived. They used a machine learning system to classify and diagnose illnesses.

Energy Efficiency Ratio (%) and Security Ratio (%)

Figure 10 shows the energy efficiency ratio (%). Since batteries power wireless sensor networks, they have high energy consumption. Nodes with power dissipation < 100 microwatts can operate longer on energy salvaged from the environment. Energy savings can be achieved by various network architecture trade-offs, including communication and sensor processors, collaborative protocols, and hierarchical networks. Battery life can be extended once the sensed data has been built using dynamic smart power techniques. For various reasons, decreasing overall power consumption is critical in WSN systems. Sensors' weight and size have mostly dictated the batteries they use. The larger the battery, the greater it is capacity. Because of this, WSN sensor nodes are particularly energy-efficient. Thus fewer batteries are used. Physiological sensors made smaller by using smaller batteries will improve user comfort. Second, long battery life is desirable since frequent battery replacements on various sensors impede user adoption. WSN operational costs were reduced as a result of increased battery life.

Figure 10. Energy efficiency ratio (%)

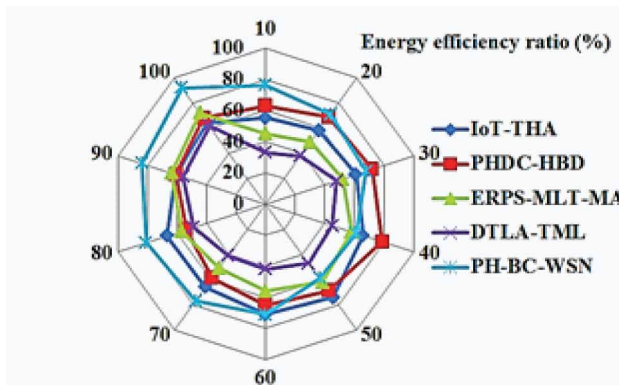


Figure 11. Security ratio (%)

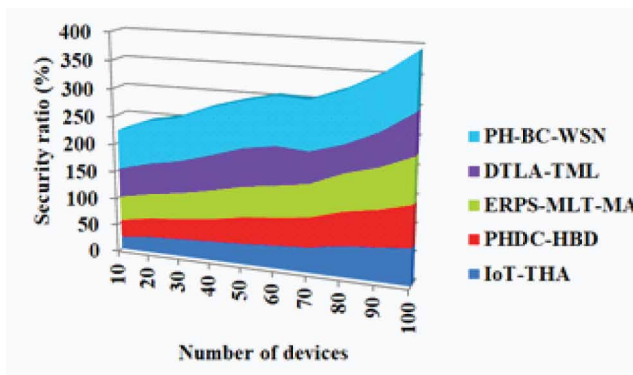



Figure 11 shows the PH-BC-WSN security ratio for a medical device. Because of the extensive implementation of the WSN algorithm, real-time monitoring has taken on new significance. Due to increased attack susceptibility, mishandling patient security and treatment procedures are increasingly commonplace in healthcare networks. To protect against this malicious attack, a PH-BC-WSN system must be built with numerous safeguards. All medical and sensor devices in a WSN network are protected by various security measures, including identity authentication and low latency. These measures include authorization management, allowing the listing of devices and password protection. Wi-Fi, Wireless, Bluetooth, and other security mechanisms are included in secure aggregation methods and verification procedures. This security is used to generate conclusions about the health of patients. PH-BC-WSN relies heavily on health security and access because of the huge amounts of data gathered and processed from a WSN of sources. Sharing these data with healthcare professionals over the server facilitates medical security actions if necessary. Users, patients, and the communication module all work together to ensure a safe and reliable transfer of information. PH-BC-WSN systems are typically used to monitor medical caretakers on a platform that enables manipulation, visualization, and health security.

These settings demonstrate that the suggested healthcare architecture effectively promotes ambulatory health services and enhances nurse monitoring. This research introduces a prototype tracking app to collect data from wireless sensors. The physical characteristics of users are gathered by the sensor network in this proposed application and then sent to electrical gadgets where they are stored in a database in a standardized manner for the foreseeable future. Using a database, a single medical professional may keep tabs on several patients. The nurse or doctor may be notified when the patient’s vital signs exceed predefined limits, for as when the heart rate or temperature rises or falls too dramatically.

Behavior Analysis Ratio (%)

Figure 12 shows that all activities done to patients who believe they are healthy to prevent or detect illness in an asymptomatic condition are referred to as preventive health behavior analysis.

Figure 12. Behavior analysis ratio (%)

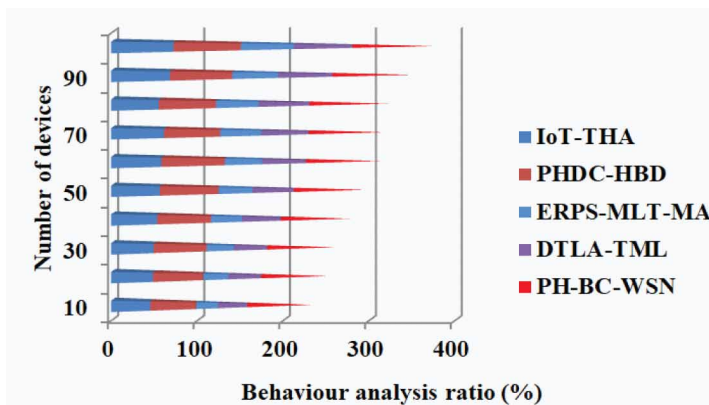

Ambulatory measurement of pulmonary function is useful for early diagnosing respiratory illnesses such as sleep apnea, COPD, and asthma and the subsequent better delivery of any necessary medications. Children with respiratory conditions benefit greatly from this round-the-clock monitoring. The monitoring system of skin sweat in patients is regarded as an essential physiologic indication

with vast potential implications for performance and human behavior. It may be interpreted differently depending on the physical activity situation and offers a new avenue for study in clinical contexts like the study of dehydration. With medical validation, the system may be trusted and utilized in or out of a clinical setting, giving the user the confidence that the data is just as reliable as that from a stationary ECG signal recorder. More data may be extracted from an ECG waveform if it is of high quality, which aids researchers in their pursuit of understanding how the heart functions normally during everyday activities.

The usage of PH-BC-WSN to promote healthy behaviors and wellness activities and the utilization of preventative treatments has increased significantly during the past decade. Health-related behavior includes preventing disease, maintaining health, improving health, and regaining health. To improve, restore, or preserve their health PH-BC-WSN is used. When designing programmers for PH-BC-WSN, accomplish good changes in health behavior, an understanding of patients and encouraging them to change. Health behavior theories and models have been established for this goal. To explain and predict a collection of events or circumstances, a theory is composed of several interrelated concepts, definitions, and propositions that together form a logical context.

Table 2. Tracking rate (%)

Number of devices	Tracking rate (%)				
	IoT-THA	PHDC-HBD	ERPS-MLT-MA	DTLA-TML	PH-BC-WSN
10	41.8	65.9	77.8	84.2	90.6
20	42.4	66.7	77.7	84.3	91.7
30	49.0	64.6	77.4	85.6	92.3
40	48.0	64.9	78.5	86.9	93.3
50	46.8	66.3	78.7	86.5	93.7
60	47.8	72.2	79.2	87.4	94.6
70	47.7	74.2	80.3	88.6	95.7
80	45.5	63.0	81.6	89.2	95.9
90	55.5	66.1	82.8	90.5	96.3
100	55.1	64.1	83.1	90.9	96.8

Table 2 shows the tracking ratio (%). Sensor devices and their usage are widely shown in the medical treatment order for patients in hospitals and other healthcare institutions. There is nothing novel about electrocardiograms and electroencephalograms; rather, they are examples of how technology and the needs of the medical system may lead to incremental improvements. Now, hospitals use PH-BC-WSN to monitor their patients' vitals, diagnose accurately, and provide effective treatments. As part of this initiative, improvements have been made to monitoring and real-time medical data inside approved zones. Within the confines of the hospital, bounded telemonitoring systems may gather real-time data from patients both in and out of the hospital's wards. Tags, which were adhered to a patient's body at all times and so were cost-effective, made it feasible to keep track of patients' medical issues during each stage (or condition) of the catastrophe. PH-BC-WSN-based patient monitoring helps keep at-risk individuals healthy and medical expenses down. PH-BC-WSN patient monitoring is a telehealth system that transmits patient information from homes, workplaces, or on the move to other healthcare practitioners. Remote care improves efficiency, health outcomes, and costs for

clinicians and patients. Efficient health management may reduce ER visits and catastrophes. Reducing hospital readmissions and increasing patient outcomes may boost Reimbursement for services and hospitals' rating system, boosting their reputation.

Few commercialized devices are currently available and have restrictions such as network configuration and configuration challenges, tracking restricted to those unable to detect catastrophe regions, inadequate installations, and connection with other systems which impacts total communication. Emergency individuals should be encouraged to track dangerous circumstances. Children and seniors with cognitive and chronic illnesses may lead safer, happier, and more independent lives.

CONCLUSION

Finally, PH-BC-WSN s can be employed in various medical settings, as demonstrated in this research. This work examines PH-BC-WSNs and the significant challenges and unresolved research concerns surrounding implantable sensors. Smaller and more multifunctional sensor nodes made possible by nanotechnology enable these new reduced body networks to become as commonplace as clothing. Researchers have been looking for ways to improve healthcare for seniors, the physically disabled, and children by incorporating new technology into existing services. In this research, we looked at real-world instances of how wireless sensor technologies might enhance people's lifetime excellence and considerations to bear in mind as these systems are designed. Wireless sensor networks are widespread, and We have investigated network data systems. For improved medical care, wireless sensor networks can achieve low-cost, energy-efficient ad-hoc installation of several sensors. With the Internet of Things, healthcare and medical asset monitoring systems can be developed more effectively. There was extensive discussion of medical data eavesdropping, manipulation, fabrication of alarms, denial of service, movement and activity monitoring of users, physical manipulation with devices, and jamming assaults. Flexibility, clean energy, and safety are some of the contemporary technology problems. Together, PH-BC-WSN is improving the healthcare system by aiding in diagnosis, sickness prognosis, drug management, and the continuous management of chronic ailments. The value of AI in enhancing the performance of IoMT and Point-of-care (POC) devices used in cutting-edge healthcare applications including heart monitoring, cancer detection, and diabetes control. A comprehensive analysis of the multiple advantages and disadvantages is included. However, with so many advantages, body sensor networks face several significant challenges and unresolved research difficulties that must be addressed. The PH-BC-WSN sensors can be added to the current setup to extend this work in the future. The experimental results show a security ratio of 92.11%, an energy efficiency ratio of 89.9%, a behavior analysis ratio of 95.23%, a tracking rate of 96.86%, a specificity ratio of 93.51% and a precision ratio of 96.8% when compared to other methods.

REFERENCES

- Abbasi, Q. H., Yang, K., Chopra, N., Jornet, J. M., Abuali, N. A., Qaraqe, K. A., & Alomainy, A. (2016). Nano-communication for biomedical applications: A review on the state-of-the-art from physical layers to novel networking concepts. *IEEE Access: Practical Innovations, Open Solutions*, 4, 3920–3935. doi:10.1109/ACCESS.2016.2593582
- Acampora, G., Cook, D. J., Rashidi, P., & Vasilakos, A. V. (2013). A survey on ambient intelligence in healthcare. *Proceedings of the IEEE*, 101(12), 2470–2494. doi:10.1109/JPROC.2013.2262913 PMID:24431472
- Albahri, A. S., Alwan, J. K., Taha, Z. K., Ismail, S. F., Hamid, R. A., Zaidan, A. A., Albahri, O. S., Zaidan, B. B., Alamoodi, A. H., & Alsalem, M. A. (2021). IoT-based telemedicine for disease prevention and health promotion: State-of-the-Art. *Journal of Network and Computer Applications*, 173, 102873. doi:10.1016/j.jnca.2020.102873
- Albahri, A. S., Alwan, J. K., Taha, Z. K., Ismail, S. F., Hamid, R. A., Zaidan, A. A., Albahri, O. S., Zaidan, B. B., Alamoodi, A. H., & Alsalem, M. A. (2021). IoT-based telemedicine for disease prevention and health promotion: State-of-the-Art. *Journal of Network and Computer Applications*, 173, 102873. doi:10.1016/j.jnca.2020.102873
- Alemdar, H., & Ersoy, C. (2010). Wireless sensor networks for healthcare: A survey. *Computer Networks*, 54(15), 2688–2710. doi:10.1016/j.comnet.2010.05.003
- Bachmann, C., Ashouei, M., Pop, V., Vidojkovic, M., De Groot, H., & Gyselinckx, B. (2012). Low-power wireless sensor nodes for ubiquitous long-term biomedical signal monitoring. *IEEE Communications Magazine*, 50(1), 20–27. doi:10.1109/MCOM.2012.6122528
- Cavaliere, L. P. L., Mangalasseri, D. K., Venkateswaran, D. P., Byloppilly, D. R., Effendy, F., More, A. B., & Regin, R. et al. (2021). The Impact Of Brand Counterfeiting on Consumer Behavior In the Fashion Sector. *Turkish Journal of Physiotherapy and Rehabilitation*, 32(3), 19831–19846.
- Cerruela García, G., Luque Ruiz, I., & Gómez-Nieto, M. Á. (2016). State of the art, trends and future of bluetooth low energy, near field communication and visible light communication in the development of smart cities. *Sensors (Basel)*, 16(11), 1968. doi:10.3390/s16111968 PMID:27886087
- Chan, M., Estève, D., Fourniols, J. Y., Escriba, C., & Campo, E. (2012). Smart wearable systems: Current status and future challenges. *Artificial Intelligence in Medicine*, 56(3), 137–156. doi:10.1016/j.artmed.2012.09.003 PMID:23122689
- Darwish, A., & Hassanien, A. E. (2011). Wearable and implantable wireless sensor network solutions for healthcare monitoring. *Sensors (Basel)*, 11(6), 5561–5595. doi:10.3390/s110605561 PMID:22163914
- Darwish, A., Hassanien, A. E., Elhoseny, M., Sangaiyah, A. K., & Muhammad, K. (2019). The impact of the hybrid platform of internet of things and cloud computing on healthcare systems: Opportunities, challenges, and open problems. *Journal of Ambient Intelligence and Humanized Computing*, 10(10), 4151–4166. doi:10.1007/s12652-017-0659-1
- Elayan, H., Shubair, R. M., & Kiourti, A. (2017, March). Wireless sensors for medical applications: Current status and future challenges. In *2017 11th European Conference on Antennas and Propagation (EUCAP)* (pp. 2478-2482). IEEE.
- Fortino, G., Di Fatta, G., Pathan, M., & Vasilakos, A. V. (2014). Cloud-assisted body area networks: State-of-the-art and future challenges. *Wireless Networks*, 20(7), 1925–1938. doi:10.1007/s11276-014-0714-1
- Fraile, J. A., Bajo, J., Corchado, J. M., & Abraham, A. (2010). Applying wearable solutions in dependent environments. *IEEE Transactions on Information Technology in Biomedicine*, 14(6), 1459–1467. doi:10.1109/TITB.2010.2053849 PMID:20667814
- Gravina, R., & Fortino, G. (2020). Wearable Body Sensor Networks: State-of-the-art and research directions. *IEEE Sensors Journal*, 21(11), 12511–12522. doi:10.1109/JSEN.2020.3044447
- Juneja, S., Kendre, S., & Patkar, U. (2016). Healthcare analysis via wireless sensor network. *IJSRSET Journal*, 2(2), 2395–1990.
- Li, K. F. (2013). Smart home technology for telemedicine and emergency management. *Journal of Ambient Intelligence and Humanized Computing*, 4(5), 535–546. doi:10.1007/s12652-012-0129-8 PMID:32218875

- Liang, T., & Yuan, Y. J. (2016). Wearable medical monitoring systems based on wireless networks: A review. *IEEE Sensors Journal*, *16*(23), 8186–8199. doi:10.1109/JSEN.2016.2597312
- Mbunge, E., Muchemwa, B., & Batani, J. (2021). Sensors and healthcare 5.0: Transformative shift in virtual care through emerging digital health technologies. *Global Health Journal*, *5*(4), 169–177. doi:10.1016/j.glohj.2021.11.008
- Ometov, A., Shubina, V., Klus, L., Skibińska, J., Saafi, S., Pascacio, P., Flueratoru, L., Gaibor, D. Q., Chukhno, N., Chukhno, O., Ali, A., Channa, A., Svrtoka, E., Qaim, W. B., Casanova-Marqués, R., Holcer, S., Torres-Sospedra, J., Casteleyn, S., Ruggeri, G., & Lohan, E. S. et al. (2021). A survey on wearable technology: History, state-of-the-art and current challenges. *Computer Networks*, *193*, 108074. doi:10.1016/j.comnet.2021.108074
- Ray, P. P., Dash, D., & Kumar, N. (2020). Sensors for internet of medical things: State-of-the-art, security and privacy issues, challenges and future directions. *Computer Communications*, *160*, 111–131. doi:10.1016/j.comcom.2020.05.029
- Rezaee, K., Savarkar, S., Yu, X., & Zhang, J. (2022). A hybrid deep transfer learning-based approach for Parkinson's disease classification in surface electromyography signals. *Biomedical Signal Processing and Control*, *71*, 103161. doi:10.1016/j.bspc.2021.103161
- Rishani, N., Elayan, H., Shubair, R., & Kiourt, A. (2018). *Wearable, epidermal, and implantable sensors for medical applications*. arXiv preprint arXiv:1810.00321.
- Saleh, Y. N., Chibelushi, C. C., Abdel-Hamid, A. A., & Soliman, A. H. (2020). *Privacy Preservation for Wireless Sensor Networks in Healthcare: State of the Art, and Open Research Challenges*. arXiv preprint arXiv:2012.12958.
- Salman, O. H., Taha, Z., Alsabah, M. Q., Hussein, Y. S., Mohammed, A. S., & Aal-Nouman, M. (2021). A review on utilizing machine learning technology in the fields of electronic emergency triage and patient priority systems in telemedicine: Coherent taxonomy, motivations, open research challenges and recommendations for intelligent future work. *Computer Methods and Programs in Biomedicine*, *209*, 106357. doi:10.1016/j.cmpb.2021.106357 PMID:34438223
- Sezer, N., & Koç, M. (2021). A comprehensive review on the state-of-the-art of piezoelectric energy harvesting. *Nano Energy*, *80*, 105567. doi:10.1016/j.nanoen.2020.105567
- Sheron, P. F., Sridhar, K. P., Baskar, S., & Shakeel, P. M. (2020, December). A decentralized scalable security framework for end-to-end authentication of future IoT communication. *Transactions on Emerging Telecommunications Technologies*, *31*(12), e3815. doi:10.1002/ett.3815
- Soh, P. J., Vandenbosch, G. A., Mercuri, M., & Schreurs, D. M. P. (2015). Wearable wireless health monitoring: Current developments, challenges, and future trends. *IEEE Microwave Magazine*, *16*(4), 55–70. doi:10.1109/MMM.2015.2394021
- Wu, W., Pirthulal, S., Sangaiah, A. K., Mukhopadhyay, S. C., & Li, G. (2018). Optimization of signal quality over comfortability of textile electrodes for ECG monitoring in fog computing based medical applications. *Future Generation Computer Systems*, *86*, 515–526. doi:10.1016/j.future.2018.04.024
- Zhang, X., & Wang, Y. (2021). Research on intelligent medical big data system based on Hadoop and blockchain. *EURASIP Journal on Wireless Communications and Networking*, *2021*(1), 1–21. doi:10.1186/s13638-020-01858-3